


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130182
Name	STEVE DUNN	ID#	4106 Date 3-15-11
A	Agency	APD	Phone # 786-2442
Instrument Location		ANCHORAGE JAIL	
Alco S/N		X172971	Target Value .084 High Pressure 500
B	Alco Test Values		.086 .087
		1st Alco	2nd Alco
Signature			
(OVER)			

BMB
4/1/11


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

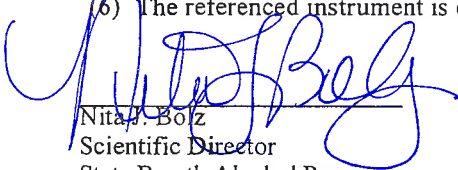
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 1ST day of APRIL, 2011.


Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

(Notary Seal Stamp)



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130182

(CONTINUED FROM FRONT PAGE)

NJB
3/17/11

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130182

MARCH 15, 2011

OPERATOR'S NAME:

DUNN/S

OPERATOR'S NUMBER: 4106

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

V

O.L. #: V

DEPT/AGENCY: ANC1

CASE/REPORT: V

TEST TYPE: V

ALCO TARGET VALUE: .084

ALCO S/N: X172971

--- BREATH ANALYSIS ---

.084 ADJUSTED FOR 29.55 in

ALCO TARGET	.082	12:31
BLANK TEST	.000	12:31
INTERNAL STANDARD	VERIFIED	12:32
ALCO TV 29.55 in	.086	12:32
BLANK TEST	.000	12:32
SUBJECT SAMPLE	.000	12:33
BLANK TEST	.000	12:34
ALCO TV 29.54 in	.087	12:34
BLANK TEST	.000	12:35

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130182

MARCH 15, 2011

TIME 12:28

--- DIAGNOSTIC CHECK ---

COMPUTER:

OKAY

PROGRAM:

OKAY

SOFTWARE DATE:

01/08/09

HEATERS

SAMPLE CHAMBER:

49c

BREATH TUBE:

42c

BAROMETER:

29.54 in

FLOW DETECTOR:

OKAY

PUMP

HIGH SPEED:

OKAY

DETECTOR:

OKAY

FILTERS:

OKAY

QUARTZ STANDARD:

OKAY

CALIBRATION:

OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnopqrstuvwxyz
pqrstuvwxyz{|}~Δ